Metrologic®

METROLOGIC INSTRUMENTS, INC.

MS7320 InVista™ Series
Installation and User's Guide

LOCATIONS

CORPORATE HEADQUARTERS

North America	Metrologic Instruments, Inc. 90 Coles Road Blackwood, NJ 08012-4683	Customer Service: 1-800-ID-METRO Tel: 856-228-8100 Fax: 856-228-6673 Email: info@metrologic.com Internet: www.metrologic.com

EUROPEAN HEADQUARTERS

Germany, **Middle East and Africa**	Metrologic Instruments GmbH Dornierstrasse 2 82178 Puchheim b. Munich, Germany	Tel: +49 89 89019 0 Fax: +49 89 89019 200 Email: info@europe.metrologic.com Germany Email: info@de.metrologic.com
Spain	Metrologic Eria Ibérica SL Julián Camarillo 29, D-1 Edificio Diapasón 28037 Madrid	Tel: +34 913 272 400 Fax: +34 913 273 829 Email: info@es.metrologic.com
Italy	Metrologic Instruments Italia srl Via Emilia 70 40064 Ozzano dell'Emilia (BO)	Tel: +39 0 51 6511978 Fax: +39 0 51 6521337 Email: info@it.metrologic.com
France	Metrologic Eria France SA 69 Rue de la Belle Etoile ZI Paris Nord II, BP 50057 95947 – ROISSY CDG CEDEX	Tel: +33 (0) 1 48.63.78.78 Fax: +33 (0) 1 48.63.24.94 Email: info@fr.metrologic.com
United Kingdom	Metrologic Instruments UK Limited 58 Tempus Business Centre Kingsclere Road, Basingstoke Hampshire RG21 6XG	Tel: +44 (0) 1256 365900 Fax: +44 (0) 1256 365955 Email: info@uk.metrologic.com

ASIA

Singapore	Metrologic Asia (Pte) Ltd No. 8 Kaki Bukit Place 4th Floor Singapore 416186	Tel: 65-6842-7155 Fax: 65-6842-7166 Email: info@sg.metrologic.com
China	Metro (Suzhou) Technologies Co., Ltd. 221 Xing Hai Street Suzhou Industrial Park Suzhou, China 215021	Tel: 86-512-62572511 Fax: 86-512-62571517 Email: info@cn.metrologic.com
Japan	Metrologic Japan Co., Ltd. Matsunoya Building, 6 Floor 3-14-8 Higashiueno Taitou-Ku, Tokyo 110-0015 Japan	Tel: 81-03-3839-8511 Fax: 81-03-3839-8519 Email: info@jp.metrologic.com

SOUTH AMERICA

Brazil	Metrologic do Brasil Ltda. Rua da Paz 2059 CEP 04713-002 Chácara Santo Antônio São Paulo, SP, Brasil	Tel: 55-11-5182-8226 Fax: 55-11-5182-8315 Email: info@br.metrologic.com
Outside Brazil	Metrologic South America Rua da Paz 2059 CEP 04713-002 Chácara Santo Antônio São Paulo, SP, Brasil	Tel: 55-11-5182-7273 Fax: 55-11-5182-7198 Email: info@sa.metrologic.com

Copyright

© 2002 by Metrologic Instruments, Inc. All rights reserved. No part of this work may be reproduced, transmitted, or stored in any form or by any means without prior written consent, except by reviewer, who may quote brief passages in a review, or provided for in the Copyright Act of 1976.

Products and brand names mentioned in this document are trademarks of their respective companies.

TABLE OF CONTENTS

Introduction 1
Scanner and Accessories 2
Installation for OCIA Interface 4
Installation for Keyboard Wedge Interface 5
Installation for Stand-Alone Keyboard Interface 6
Installation for USB Interface 7
Installation for RS232 or Light Pen Interfaces 8
Installation for IBM 46xx Interface 10
Installation of an Auxiliary Scanner 11
Scanner Parts 14
Maintenance 14
Cable Cover Installation and Removal 15
Face Plate Removal 15
Scanner Labels 16
Audible Indicators 17
Visual Indicators 18
Failure Modes 19
Power Save Modes and the Multi-Function Button 20
Scan Volume 22
Depth of Field by Minimum Bar Code Element Width 23
Flex Stand Installation 25
EAS Deactivation Antenna 27
Troubleshooting Guide 28
Design Specifications 33
RS232 Demonstration Program 35
Applications and Protocols 36
Default Settings 37
Scanner and Cable Terminations 43
Limited Warranty 47
Notices 48
Patents 50
Index 51

INTRODUCTION

The MS7320 InVista™ offers an outstanding combination of features, versatility, performance, and durability. This fixed mount laser bar code scanner provides ease of use and high throughput speeds by featuring a large, dynamic, and aggressive scan volume.

The MS7320 is equipped with a multitude of standard features including:

- Automatic scanning operation
- Firmware updates via Flash ROM
- EAS deactivation antenna
- A Programmable Depth of Field
- Supports multiple interfaces including USB and Keyboard Wedge
- Custom edit the bar code data
- OPOS and JPOS system compatible
- RS232 auxiliary port for adding peripherals
- PowerLink, user replaceable cables
- Field replaceable outer window

SCANNER	INTERFACE
MS7320-**13**	RS232, IBM 46xx, OCIA, Aux
MS7320-**37**	RS232, Light Pen, Keyboard Wedge, Stand-Alone Keyboard, USB, Aux

SCANNER AND ACCESSORIES

BASIC KIT	
Part #	**Description**
MS7320	InVista Series Scanner
00-02407A-1 & 00-02407A-2	MetroSelect® Programming Guide Two Book Set
00-02896	MS7320 InVista Series Installation and User's Guide
52-52511A	24" EAS Cable

Guides also available for download at www.metrologic.com.

OPTIONAL ACCESSORIES	
Part #	**Description**
54-54xxx*	Straight PowerLink Cable with built in power jack. 2.1 m (7') cord with short strain relief
xxx specifies connection to the host.* *Contact a customer service representative for additional information.*	
54-54002	Keyboard Wedge PowerLink Cable with Adapter Cable
MVC**	Metrologic Voltage Converter Cable, +12VDC to +5.2VDC or -12VDC to +5VDC
** *Contact a Metrologic Customer Service representative for additional information on Metrologic's MVC cable series and the host connections available.*	
54-54020	Stand Alone Keyboard Wedge PowerLink Cable
54-54165	USB PowerLink Cable (Type A)
54-54667	RS232 AUX PowerLink Cable

OPTIONAL ACCESSORIES	
Part #	**Description**
AC to DC Power Transformer - Regulated 5.2V@650 mA output	
45-45593	120V United States
45-45591	220V – 240V Continental European
45-45592	220V – 240V United Kingdom
45-45483	Flex Stand

REPLACEMENT PARTS	
Part #	**Description**
46-46624	Everscan Window Face Plate
46-46625	Standard Window Face Plate

Other items may be ordered for the specific protocol being used. To order additional items, contact the dealer, distributor or call Metrologic's Customer Service Department at 1-800-ID-METRO or 1-800-436-3876.

1. Turn off the host system.

2. Connect the MVC cable to the 10-pin OCIA interface jack. It is the 2nd ***round*** opening from the left side of the MS7320 (*see figure 1*).

3. Connect the other end of the MVC cable to the host.

STOP Before continuing verify that the MVC cable is connected to the appropriate interface jack on the scanner. An incorrect cable connection can cause communication problems or potential damage to the scanner.

Plugging the scanner into the serial port of the PC does not guarantee that scanned information will appear at the PC. A software driver and correct configuration settings are also required for proper communication.

4. Turn on the host system.

5. Scan the *Load OCIA Defaults* bar code to configure the MS7320 for OCIA communication.

6. Snap on the cable cover.

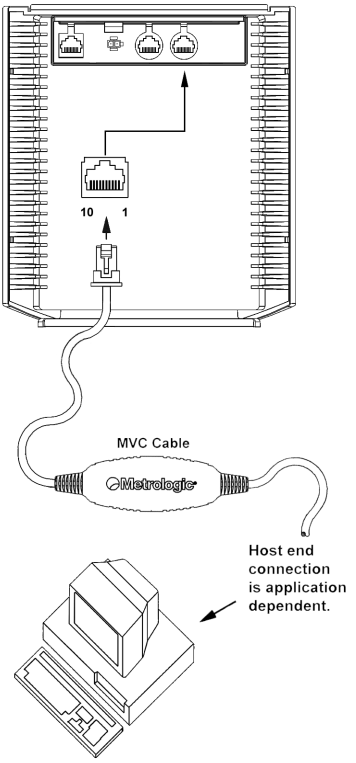

Figure 1: *OCIA, Interface*

Load OCIA Defaults



For additional communication options for OCIA interfaces refer to the *MetroSelect Programming Guide* (MLPN 00-02407A-1 & -2).

Caution:
To maintain compliance with applicable standards, all circuits connected to the scanner must meet the requirements for SELV (Safety Extra Low Voltage) according to EN 60950.

To maintain compliance with standard CSA C22.2 No. 60950-00/UL 60950 and norm EN 60950, the power source should meet applicable performance requirements for a limited power source.

INSTALLATION FOR KEYBOARD WEDGE INTERFACE

1. Turn off the host system.
2. Disconnect the keyboard from the host.
3. Connect the PowerLink cable to the 10-pin KBW interface jack. It is the 2nd ***round*** opening from the left side of the MS7320 *(see figure 2).*
4. Connect the "Y" end of the PowerLink cable to the keyboard and the keyboard port on the host. If necessary use the male/female adapter cable supplied with the scanner for proper connections.

STOP Before continuing verify that the PowerLink cable is connected to the appropriate interface jack on the scanner. An incorrect cable connection can cause communication problems or potential damage to the scanner.

5. Connect the external power supply to the power jack on the PowerLink cable.
6. Check the AC input requirements of the power supply to make sure the voltage matches the AC outlet.
7. Connect AC power to the transformer. The outlet should be near the equipment and easily accessible.
8. Scan the *Load Keyboard Wedge Defaults* bar code to configure the MS7320 for Keyboard Wedge communication.
9. Turn on the host system.
10. Snap on the cable cover.

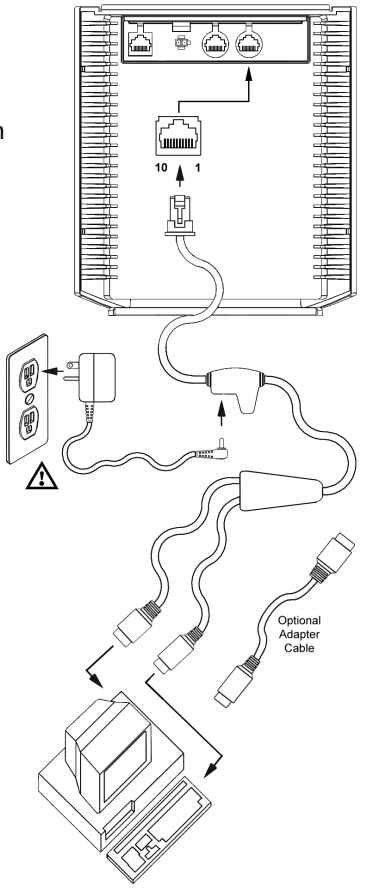

Figure 2: *Keyboard Wedge Interfaces*

Load Keyboard
Wedge Defaults

Caution:
To maintain compliance with applicable standards, all circuits connected to the scanner must meet the requirements for SELV (Safety Extra Low Voltage) according to EN 60950.

To maintain compliance with standard CSA C22.2 No. 60950-00/UL 60950 and norm EN 60950, the power source should meet applicable performance requirements for a limited power source.

INSTALLATION FOR STAND-ALONE KEYBOARD INTERFACE

1. Turn off the host system.
2. Disconnect the keyboard from the host.
3. Connect the PowerLink cable to the 10-pin Stand-Alone Keyboard interface jack. It is the 2nd ***round*** opening from the left side of the MS7320 *(see figure 3)*.
4. Connect the other end of the PowerLink cable to the keyboard port on the host.

STOP Before continuing verify that the PowerLink cable is connected to the appropriate interface jack on the scanner. An incorrect cable connection can cause communication problems or potential damage to the scanner.

5. Connect the external power supply to the power jack on the PowerLink cable.
6. Check the AC input requirements of the power supply to make sure the voltage matches the AC outlet.
7. Connect AC power to the transformer. The outlet should be near the equipment and easily accessible.
8. Scan the two bar codes in numbered sequence in order to configure the MS7320 for Stand-Alone Keyboard communication.

   Note:
   When scanning the bar codes, cover the code not being scanned to ensure the codes are read in the proper sequence.
9. Turn on the host system.
10. Snap on the cable cover.

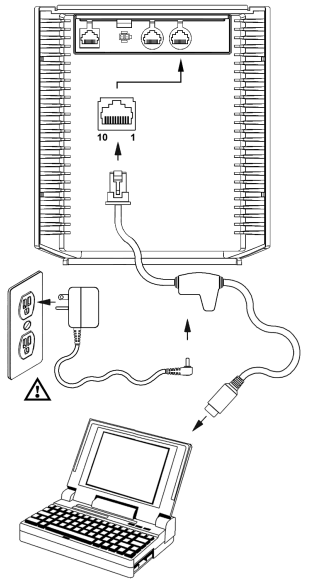

Figure 3: *Stand-Alone Keyboard Interface*

Load Keyboard Wedge Defaults

Scan 1St

Enable Stand-Alone Keyboard Wedge

Scan 2nd

Caution:
To maintain compliance with applicable standards, all circuits connected to the scanner must meet the requirements for SELV (Safety Extra Low Voltage) according to EN 60950.

To maintain compliance with standard CSA C22.2 No. 60950-00/UL 60950 and norm EN 60950, the power source should meet applicable performance requirements for a limited power source.

INSTALLATION FOR USB INTERFACE

1. Turn off the host system.
2. Determine if your application requires **USB Keyboard** communication protocols or **USB Point-of-Sale** communication protocols.
3. If you require **USB Keyboard** communication protocols, **skip** to step 4.

   If you require **USB Point-of-Sale** communication protocols set the dip switches shown in *figure 4a* to positions 1 and 2.
4. Connect the PowerLink cable to the 10-pin USB interface jack. It is the 2nd ***round*** opening from the left side of the MS7320 *(see figure 4b)*.
5. Connect the other end of the USB cable to the host.

STOP Before continuing verify that the USB cable is connected to the appropriate interface jack on the scanner. An incorrect cable connection can cause communication problems or potential damage to the scanner.

Plugging the scanner into the USB port of the PC does not guarantee that scanned information will appear at the PC. A software driver and correct configuration setting are also required for proper communication.

6. Scan the *Enable USB Defaults* bar code to configure the MS7320 for USB communication.
7. Turn on the host system.
8. Snap on the cable cover.

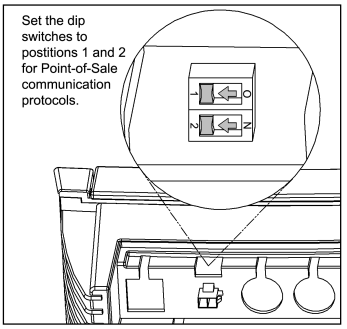

Figure 4a: *POS Dip Switch*

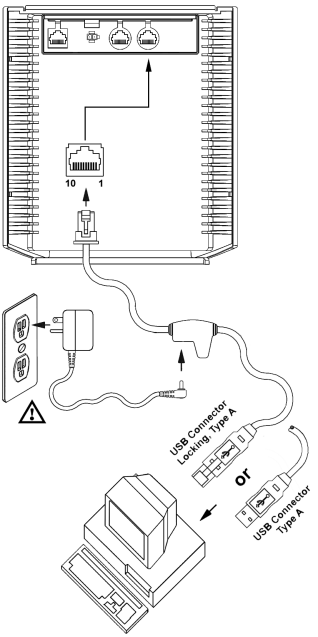

Figure 4b: *USB, Interface*

Enable USB Defaults

Caution: To maintain compliance with applicable standards, all circuits connected to the scanner must meet the requirements for SELV (Safety Extra Low Voltage) according to EN 60950.

To maintain compliance with standard CSA C22.2 No. 60950-00/UL 60950 and norm EN 60950, the power source should meet applicable performance requirements for a limited power source.

INSTALLATION FOR RS232 OR LIGHT PEN INTERFACES

1. Turn off the host system.

2. Connect the PowerLink cable to the 10-pin RS232/Light Pen interface jack. It is the 1st ***round*** opening from the left side of the MS7320 *(see figure 5).*

3. Connect the other end of the PowerLink cable to the host.

STOP Before continuing verify that the PowerLink cable is connected to the appropriate interface jack on the scanner. An incorrect cable connection can cause communication problems or potential damage to the scanner.

4. Connect the external power supply to the power jack on the PowerLink Cable.

5. Check the AC input requirements of the power supply to make sure the voltage matches the AC outlet.

6. Connect AC power to the transformer. The outlet should be near the equipment and easily accessible.

7. Scan the appropriate bar codes on page 9 to configure the MS7320 for RS-232 or Light Pen communication.

8. Turn on the host system.

9. Snap on the cable cover.

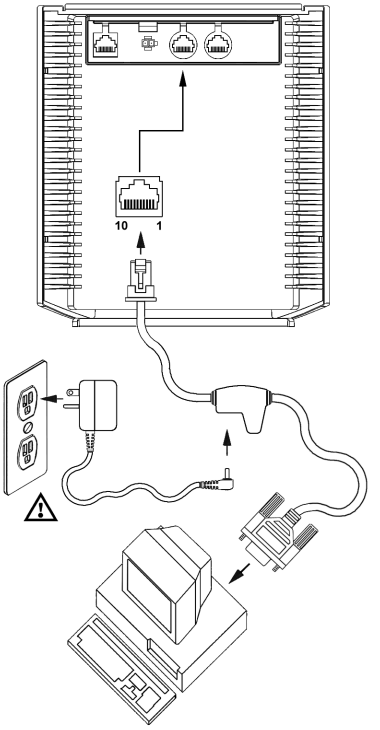

Figure 5: *RS232 or Light Pen Interface*

Caution:
To maintain compliance with applicable standards, all circuits connected to the scanner must meet the requirements for SELV (Safety Extra Low Voltage) according to EN 60950.

To maintain compliance with standard CSA C22.2 No. 60950-00/UL 60950 and norm EN 60950, the power source should meet applicable performance requirements for a limited power source.

INSTALLATION FOR RS232 OR LIGHT PEN INTERFACES

Codes needed for Step 7 on page 8.

For RS232 Communication:

Recall Defaults

Scan 1st

Enable RS-232

Scan 2nd

For Light Pen Communication:

Recall Defaults

Scan 1st

Enable Light Pen/Wand

Scan 2nd

1. Turn off the host system.

2. Connect the MVC cable to the 10-pin IBM 46xx interface jack. It is the 1st ***round*** opening from the left side of the MS7320 *(see figure 6)*.

3. Connect the other end of the MVC cable to the host.

STOP Before continuing verify that the MVC cable is connected to the proper communication jack on the scanner. Incorrect cable connection can cause communication problems or potential damage to the scanner.

Plugging the scanner into the serial p that scanned information will appear correct configuration setting are also communication to occur.

4. Turn on the host system.

5. Scan the *Load 46xx IBM Defaults* bar code to configure the MS7320 for RS232/IBM communication.

6. Snap on the cable cover

For additional communication options for IBM interfaces refer to the MetroSelect Programming Guide (MLPN 00-02407A-1 & -2).

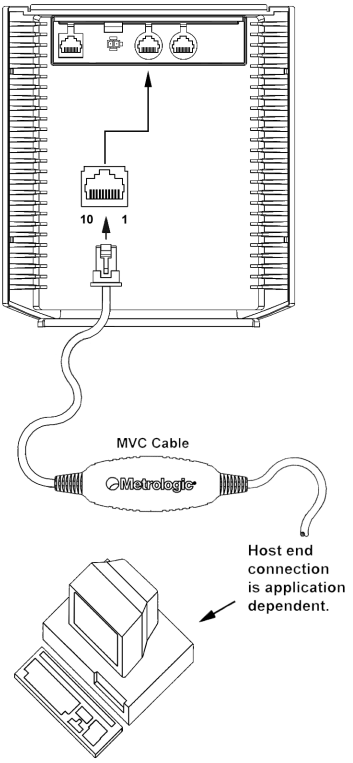

Figure 6: *IBM 46xx Interface*

Load 46xx IBM Defaults

Caution:
To maintain compliance with applicable standards, all circuits connected to the scanner must meet the requirements for SELV (Safety Extra Low Voltage) according to EN 60950.

To maintain compliance with standard CSA C22.2 No. 60950-00/UL 60950 and norm EN 60950, the power source should meet applicable performance requirements for a limited power source.

INSTALLATION OF AN AUXILIARY SCANNER

1. Turn off the host system.

2. Connect the round end of the *PowerLink RS232 AUX* cable [MLPN 54-54667A] to the RS232 jack of the auxiliary scanner (*see figure 7*).

3. Connect the other end of the *PowerLink RS232 AUX* cable into the 1st jack from the left side of the MS7320. The Aux jack has a ***square*** opening.

   The following Metrologic scanners can be used in the "Aux" input of the MS7320: the MS9520, MS9540, MS6220, MS7120, MS6520, MS6720, MS7220 or another MS7320.

   Important: The MS7320 aux port requires the signals: transmit, receive, RTS & CTS from the auxiliary scanner.

4. Connect the MS7320/Host PowerLink* cable to the appropriate interface jack on the back of the MS7320.

5. Connect the other end of the MS7320/Host PowerLink cable to the Host.

6. Connect the external power supplies for the auxiliary scanner and the MS7320 to the power jacks on the two PowerLink cables.

   STOP Before continuing verify that the PowerLink cables are connected to the appropriate interface jacks on the scanner. An incorrect cable connection can cause communication problems or potential damage to the scanner.

7. Check the AC input requirements of both power supplies to make sure the voltage matches the AC outlets.

8. Snap on the cable cover.

9. Connect AC power to the transformers. The outlets should be near the equipment and easily accessible.

10. Configure the MS7320 for the appropriate interface configuration settings.*

Continued on page 12.

* The MS7320/host cable connection is interface dependent. Refer to the installation steps provided for the type of interface required for your application.

Caution:
To maintain compliance with applicable standards, all circuits connected to the scanner must meet the requirements for SELV (Safety Extra Low Voltage) according to EN 60950.

To maintain compliance with standard CSA C22.2 No. 60950-00/UL 60950 and norm EN 60950, the power source should meet applicable performance requirements for a limited power source.

11. Configure the **auxiliary scanner** to send formatted data to the MS7320. Normal slave mode operation will only require reserve Code 32 to be set in the auxiliary scanner. The following bar code applies for all scanners, **except the MS6720**, to be used as an auxiliary scanner. Contact a Metrologic representative for additional information on the MS6720.

Reserve Code 32



Metrologic recommends disabling the beeper on the auxiliary scanner. Refer to 'Beeper Options' in the Communications section of the MetroSelect Configuration Guide (MLPN 00-02407A-1 & -2).

12. Configure the MS7320 to activate the auxiliary port. Enable the auxiliary port and configure it to recognize slave formatted data with the following bar code:

Enable Aux Port



13. Turn on the host system.

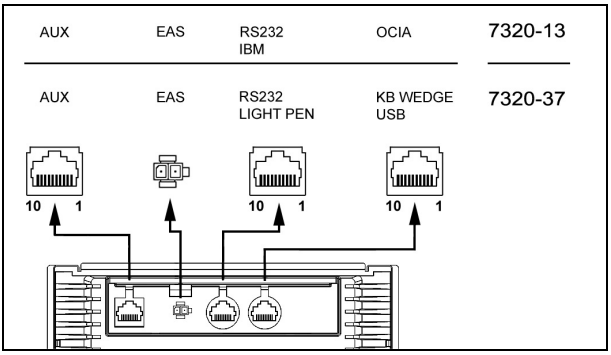

Figure 7: *Connector Orientation (Top)*
Auxiliary Scanner Setup (Bottom)

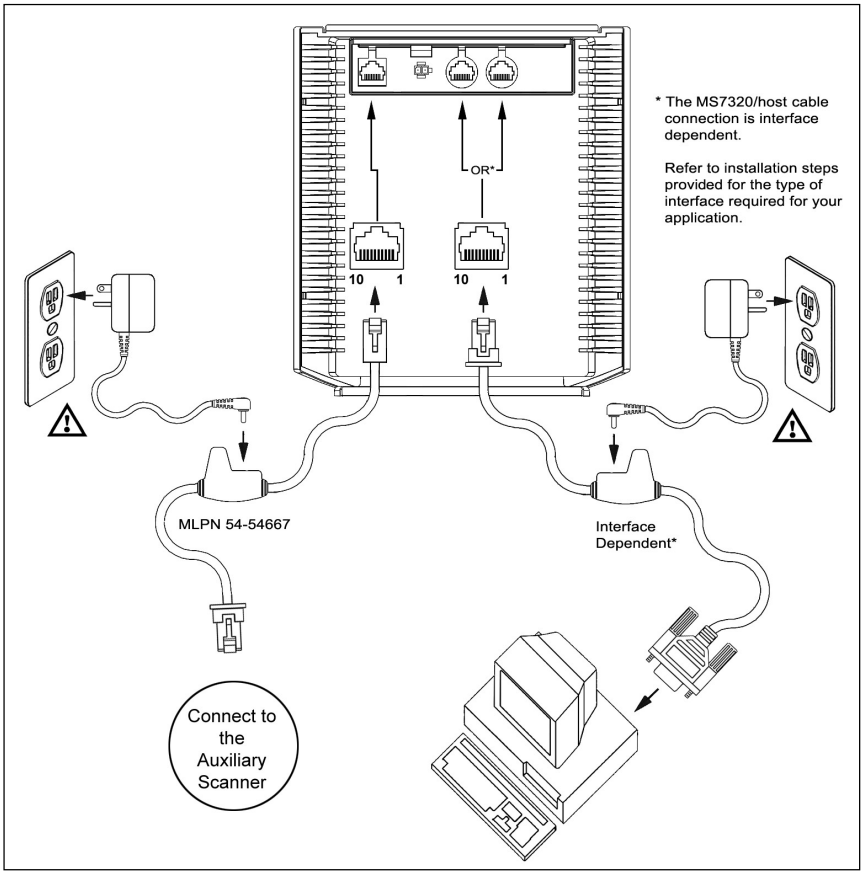
OR*
10 1
10 1
* The MS7320/host cable connection is interface dependent.
Refer to installation steps provided for the type of interface required for your application.
MLPN 54-54667
Interface Dependent*
Connect to the Auxiliary Scanner

SCANNER PARTS

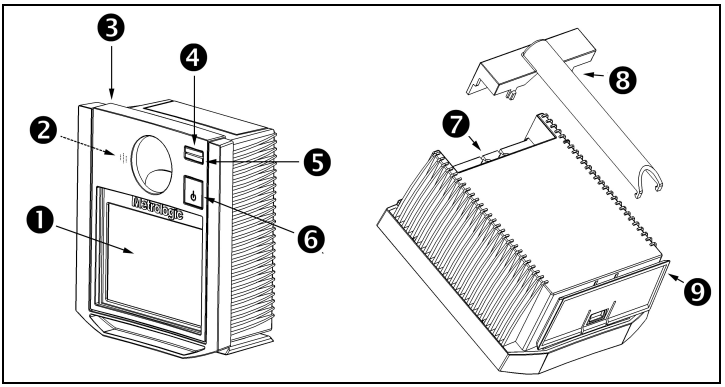

Figure 8: *Scanner Parts*

❶ Output Window (Laser Aperture)

❷ Speaker (Under the Window Cover)

❸ Replaceable Window Face Plate

❹ Red LED *(Top LED)*

❺ Green LED *(Bottom LED)*

❻ Muli-Function Button *(see page 20)*

❼ Cable Connection and Dip Switch Area

❽ Cable Cover

❾ Stand Foot

MAINTENANCE

Smudges and dirt can interfere with the proper scanning of a bar code. Therefore, the output window will need occasional cleaning.

For the MS7320 glass window:

1. Spray glass cleaner onto lint free, non-abrasive cleaning cloth.
2. Gently wipe the scanner window.

For the MS7320 red window:

1. Use mild soap and water with lint free, non-abrasive cleaning cloth.
2. Gently wipe the scanner window.

CABLE COVER INSTALLATION AND REMOVAL

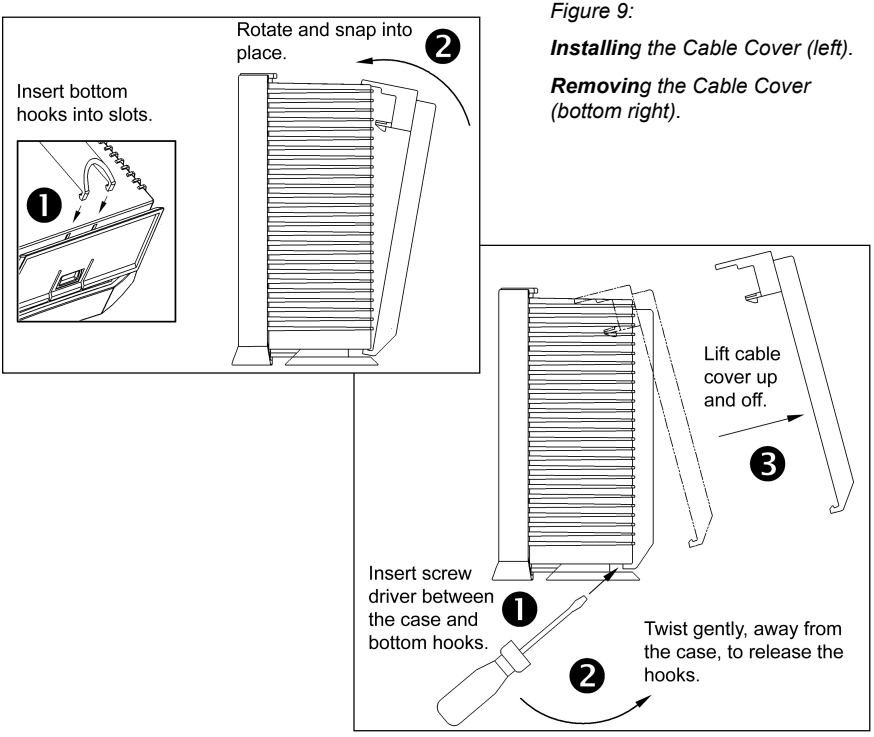
Rotate and snap into place.
2
Insert bottom hooks into slots.
1
Lift cable cover up and off.
3
Insert screw driver between the case and bottom hooks.
1
Twist gently, away from the case, to release the hooks.
2

Figure 9:

***Installing** the Cable Cover (left).*

***Removing** the Cable Cover (bottom right).*

FACE PLATE REMOVAL

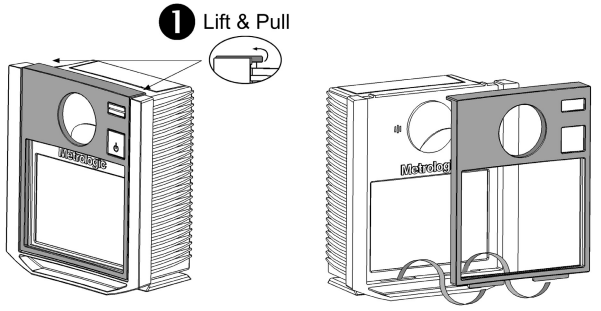

***Figure 10:** Face Plate Removal*

SCANNER LABELS

The MS7320 has 2 labels on the back of the unit. These labels contain the model number, date of manufacture, serial number, and caution information. An additional caution label is located under the *window faceplate* and a label noting the jack interfaces is located under the connector cover. The following are examples of these labels.

Figure 11: *Scanner Labels*

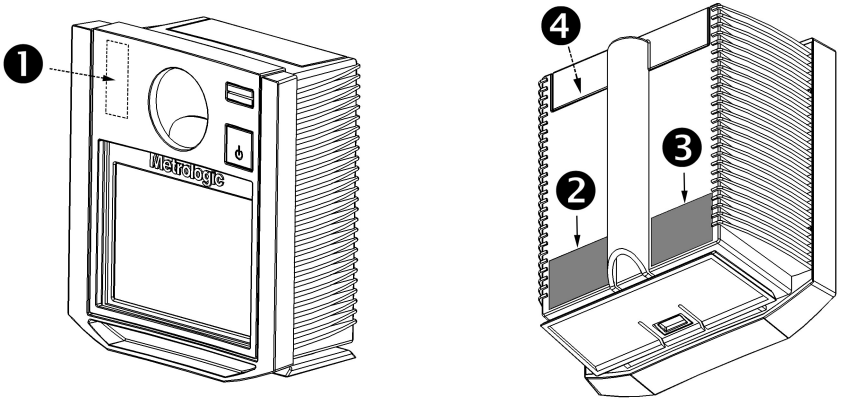

1

CAUTION - CLASS 2 LASER LIGHT WHEN OPEN.
DO NOT STARE INTO BEAM. ATTENTION - CLASSE 2
RAYONNEMENT LASER EN CAS D'OUVERTURE. NE PAS
REGARDER DANS LE FAISCEAU.

2

Metrologic Instruments, Inc.
Blackwood, New Jersey, U.S.A
Manufactured: January 2002 (P) 13
Blackwood, NJ, U.S.A. 5V ⎓
InVista™ Barcode Scanner
Model: MS7320 IBM/OCIA/RS232
4302030019
This Product is covered by one or more patents. See Users' Guide for complete patent list.

Contains no user serviceable components.
Complies with 21 CFR 1040.10 and 1040.11 except deviations pursuant to Laser Notice No. 50 dated July 26, 2001.

Patents See Manual.

3

CAUTION - CLASS 2 LASER LIGHT WHEN OPEN.
DO NOT STARE INTO BEAM. ATTENTION - CLASSE 2
RAYONNEMENT LASER EN CAS D'OUVERTURE. NE PAS
REGARDER DANS LE FAISCEAU.

IEC 60825-1:1993 + A2:2001

CLASS 1 LASER PRODUCT
APPAREIL A LASER DE
CLASSE 1

LASER KLASSE 1
PRODUKT

4

AUX	EAS	RS232 IBM	OCIA	7320-13
AUX	EAS	RS232 LIGHT PEN	KB WEDGE USB	7320-37

See serial number label for applicable interfaces.

AUDIBLE INDICATORS

When the MS*7320* scanner is in operation, it provides audible feedback. These sounds indicate the status of the scanner. Eight settings are available for the tone of the beep (normal, 6 alternate tones and no tone). To change the tone, use the *Multi-Function Button* or refer to the MetroSelect® Programming Guide.

One Beep

When the scanner *first* receives power, the green LED will turn on, the red LED will flash and the scanner will beep once. (The red LED will remain on for the duration of the beep.) The scanner is now ready to scan.

When the scanner *successfully* reads a bar code, the red LED will flash and the scanner beeps once (if programmed to do so). If the scanner does not beep once and the red light does not flash, then the bar code has *not* been successfully read.

Razzberry Tone

This is a failure indicator. Refer to failure modes page 19.



Three Beeps - during operation

When placing the scanner in program mode, the red LED will flash while the scanner simultaneously beeps three times. The red and green LEDs will continue to flash until the unit exits program mode. Upon exiting program mode, the scanner will beep three times and the red LED will stop flashing.

When configured, 3 beeps can also indicate a communications timeout during normal scanning mode.

When using one-code-programming, the scanner will beep three times (the current selected tone), followed by a short pause, a high tone and a low tone. This tells the user that the single configuration bar code has *successfully* configured the scanner.

Three beeps will also occur during a manual adjustment of the beeper tone. With each short depression of the *Multi-Function Button*, the new tone will be heard, followed by a short pause then two more of the new current tones.



Three Beeps - on power up

This is a failure indicator. Refer to failure modes page 19.

There is a red LED and green LED on the front of the MS*7320*. When the scanner is on, the flashing or constant illumination of the LEDs indicates the status of the current scan and the scanner.



Figure 12: *LEDs*

No Red or Green LED

The LEDs will not be illuminated if the scanner is not receiving power from the host or transformer.

Steady Green

When the laser is active, the green LED is illuminated. The green LED will remain illuminated until the laser is deactivated.

During the power save mode, the laser will turn on and off. During this period, the green LED remains illuminated.

Steady Green and Single Red Flash

When the scanner successfully reads a bar code, the red LED will flash and the scanner will beep once. If the red LED does not flash or the scanner does not beep once, then the bar code has not been successfully read.

Steady Green and Steady Red

After a successful scan, the scanner transmits the data to the host device. Some communication modes require that the host inform the scanner when data is ready to be received. If the host is not ready to accept the information, the scanner's red LED will remain on until the data can be transmitted.



Flashing Green then Flashing Red

This indicates the scanner is in program mode. A razzberry tone indicates that an invalid bar code has been scanned in this mode.

or

If the unit is in sleep mode, each LED will flash once every 15 seconds.

Steady Red, Green off

This indicates the scanner may be waiting for communication from the host.



Figure 13: *LEDs*



Flashing Green and One Razzberry Tone

This indicates the scanner has experienced a laser subsystem failure. Return the unit for repair at an authorized service center.



Flashing Red and Green and Two Razzberry Tones

This indicates the scanner has experienced a motor failure. Return the unit for repair at an authorized service center.



Continuous Razzberry Tone with both LEDs off

If, upon power up, the scanner emits a continuous razzberry tone, then the scanner has an electronic failure. Return the unit for repair at an authorized service center.



Three Beeps - on power up

If the scanner beeps 3 times on power up then, the nonvolatile memory that holds the scanner configuration has failed. Return the unit for repair at an authorized service center.

POWER SAVE MODES AND THE MULTI-FUNCTION BUTTON

The MS*7320* has five programmable power save modes. Refer to the *MetroSelect Programming Guide* for additional information on Power Save Modes.

1. **Blink Power Save Mode (Default):**
   "Blinks" the laser OFF & ON after a programmed period of non-use.

   When the scanner recognizes a bar code it will exit the Blink mode.

2. **Laser Off Power Save Mode:**
   Turns the laser OFF after a programmed period of non-use.

   The motor continues to spin allowing for a faster "wake" up time. Pressing the Multi-Function button will "wake" the scanner from the *Laser Off* power save mode (see figure 17).

3. **Laser & Motor Off Power Save Mode:**
   Turns the laser and motor OFF after a programmed period of non-use.

   Pressing the Multi-Function button will "wake" the scanner from the power save mode (see figure 17). This mode is the only power save mode that can be activated by the Multi-Function Button (see figure 16). This mode's "wake up" time is slightly longer due to the motor's need to restart.

4. **Dual Action Power Save Mode #1:**
   "Blinks" the laser OFF & ON after a programmed period of non-use turns the laser and motor OFF at thirty-minute intervals.

   Example:
   If the power save timeout is set to 15 minutes.

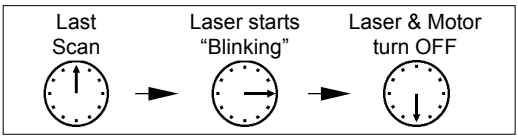

   Pressing the Multi-Function button will "wake" the scanner from the power save mode (see figure 17).

5. **Dual Action Power Save Mode #2:**
   Turns the laser OFF after a programmed period of non-use then turns the motor OFF after thirty-minute intervals.

   Example:
   If the power save timeout is set to 15 minutes.

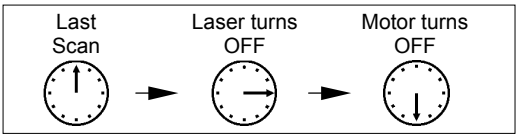

   Pressing the Multi-Function button will "wake" the scanner from the power save mode (see figure 17).



Figure 14: *The Multi-Function Button*

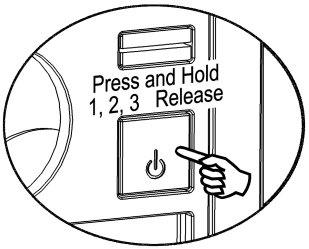

Figure 15: *Changing the Beeper Tone*

CHANGING THE BEEPER TONE

A short (<3 second) depression and the beeper tone will change. The new tone will be heard, followed by a short pause. Then two more of the new tones will be heard signifying the new setting has been stored in memory. The silent (no beep) tone is also selectable.

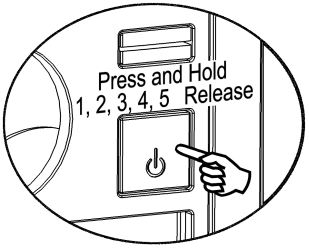

Figure 16: *Laser & Motor Off Power Save Mode*

PLACING THE UNIT IN LASER & MOTOR OFF POWER SAVE MODE

Long (>3 seconds) depression
The *Laser & Motor Off Power Save Mode* is the only power save mode that can be activated with the multi-function button.

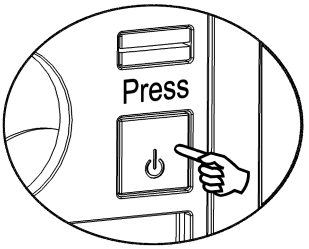

Figure 17: *Normal Operation*

WAKING THE UNIT FROM ALL POWER SAVE MODES

The next button depression will awaken the scanner for normal operation.

SCAN VOLUME

(BASED ON 100% UPC BAR CODES)

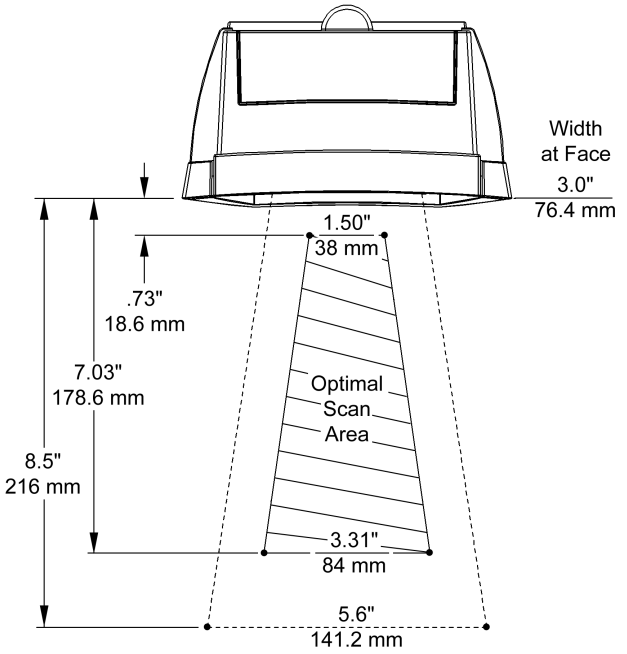

Figure 18: *Scan Area Top View (top) Side View (Bottom)*

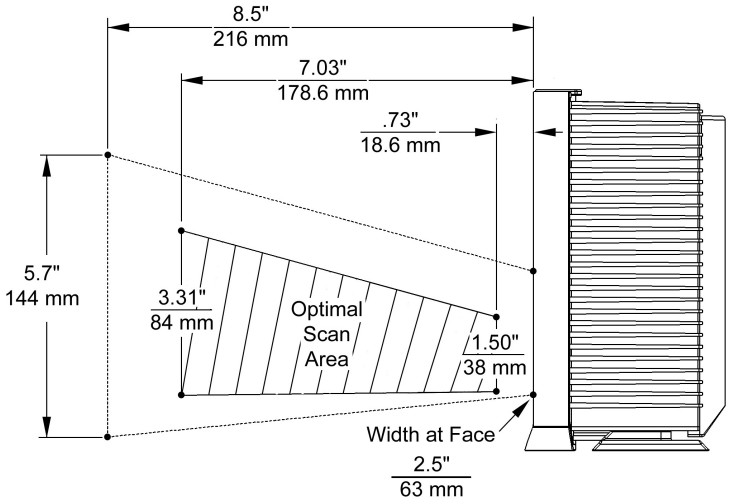

Specifications subject to change without notice.

DEPTH OF FIELD BY MINIMUM BAR CODE ELEMENT WIDTH

(BASED ON 100% UPC BAR CODES)

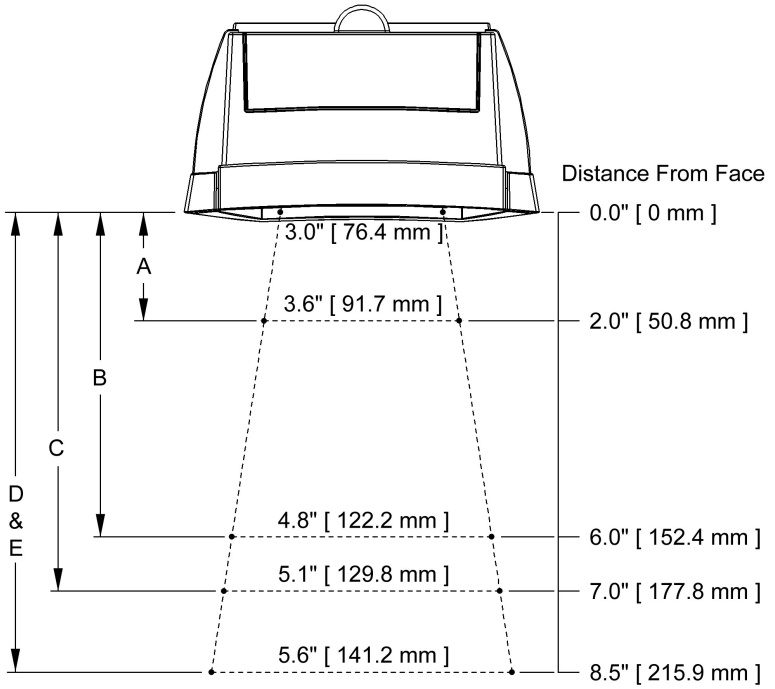

Figure 19: *Depth of Field Top View*

	Minimum Bar Code Element Width				
	A	**B**	**C**	**D**	**E**
mm	.13	.19	.26	.33	.48
mils	5.2	7.5	10.4	13	19

Specifications subject to change without notice.

DEPTH OF FIELD BY MINIMUM BAR CODE ELEMENT WIDTH

(BASED ON 100% UPC BAR CODES)

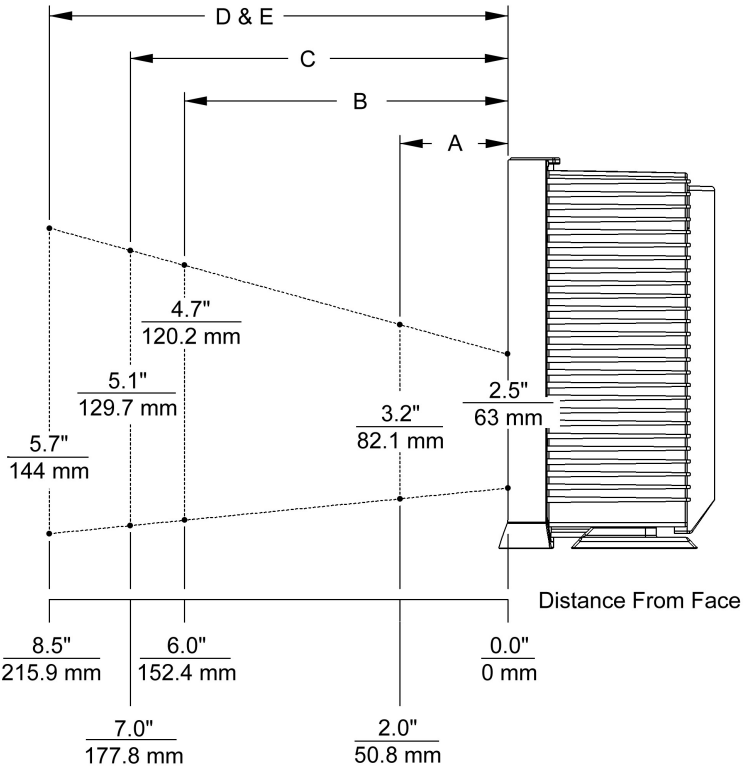

Figure 20: *Depth of Field Side View*

	Minimum Bar Code Element Width				
	A	**B**	**C**	**D**	**E**
mm	.13	.19	.26	.33	.48
mils	5.2	7.5	10.4	13	19

Specifications subject to change without notice.

The Optional Flex Stand (MLPN 45-45483) includes:

a. Shoe Mount .....Qty. 1
b. Stand Base Cover .....Qty. 1
c. Stand Base.....Qty. 1
d. Small Flex Cover .....Qty. 1
e. Flex Pole .....Qty. 1
f. Large Flex Cover.....Qty. 1
g. #8 x 1.00” Wood Screw.....Qty. 4
h. ¼”-20 x ¾” Flat Head Screw .....Qty. 1
i. #4-40 x ⅜” Phillips Head Screw ...Qty. 1
j. ¼” Internal Lock Washer.....Qty. 1

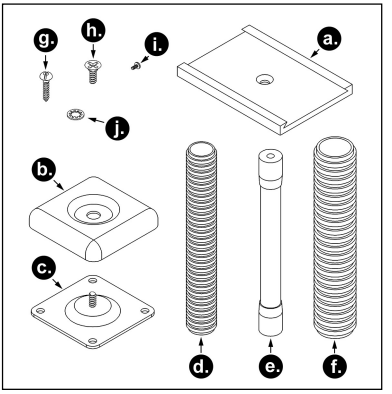

Figure 21: *Scanner Parts*

Installation

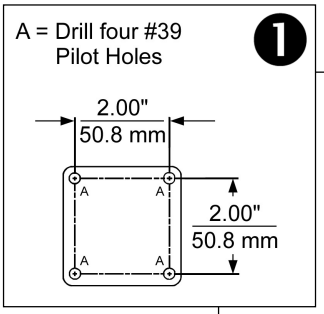

Figure 22

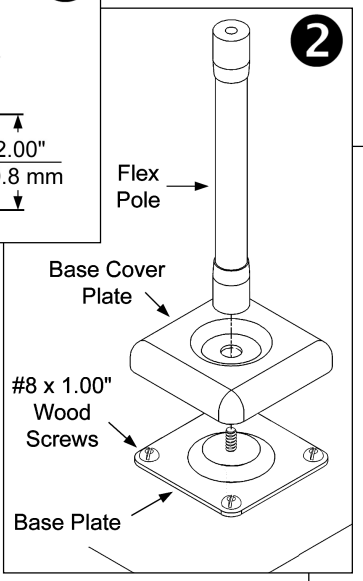

Figure 23

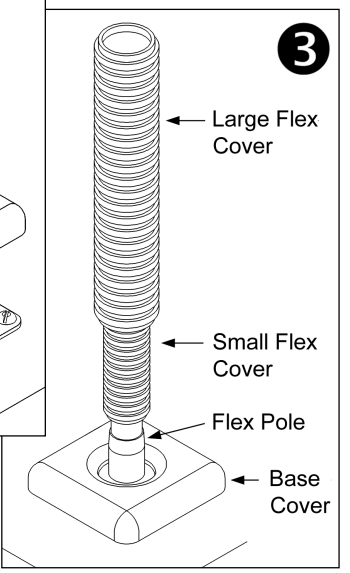

Figure 24

Optional Flex Stand (MLPN 45-45483) installation continued from page 25.

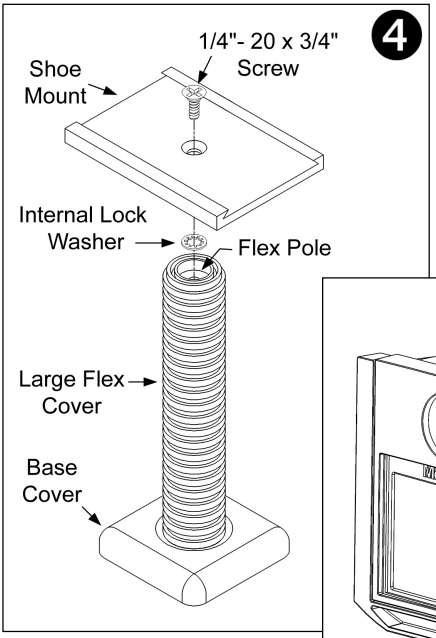

Figure 25

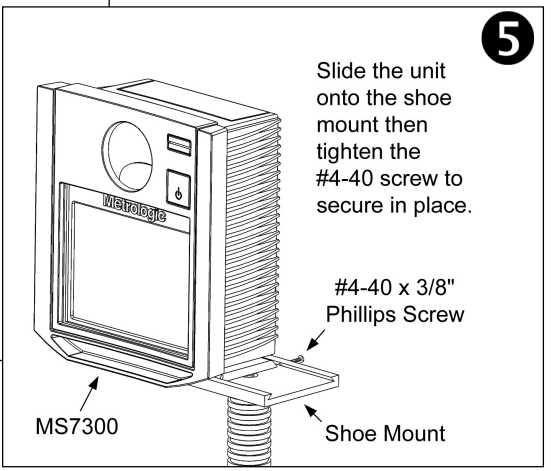

Figure 26

EAS DEACTIVATION ANTENNA

SW1 and SW2 are the switch banks inside the Checkpoint Device that set the deactivation range. Metrologic recommends end users program the MS7320 to the Fixed Low-Density depth of field, so that the unit does not scan out beyond the deactivation range.

Unit #	CheckPoint Recommended Switch Bank Settings	MS7320 Depth of Field Settings
MS**7320**	2, 3, 4, 5, 6 on SW1 & SW2	Default
**Note: Minimum element width changes to 6.8 mil when in this mode.*		

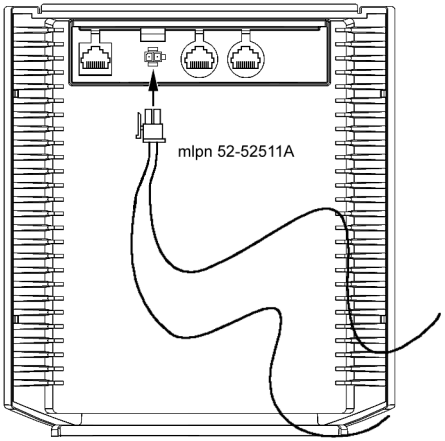

Figure 27: *EAS Deactivation Antenna*

Contact Checkpoint Systems directly for additional EAS support

TROUBLESHOOTING GUIDE

The following guide is for reference purposes only. Contact a Metrologic representative at 1-800-ID-METRO or 1-800-436-3876 to preserve the limited warranty terms.

MS7320 SERIES TROUBLESHOOTING GUIDE		
SYMPTOMS	**POSSIBLE CAUSE(S)**	**SOLUTION**
All Interfaces		
No LEDs, beep or motor spin.	No power is being supplied to the scanner.	Check transformer, outlet and power strip. Make sure the cable is plugged into the scanner.
No LEDs, beep.	No power is being supplied to the scanner from host.	Some host systems cannot supply enough current to power MS7320 series scanner. Use the power supply included with the scanner.
3 beeps on power up.	Non-volatile RAM failure.	Contact a Metrologic Representative, if the unit will not hold the programmed configuration.
Continuous razz tone on power up.	RAM or ROM failure.	Contact a Metrologic Representative, if the unit will not function.
Razz tone and green LED flash at power up.	VLD failure.	Contact a Metrologic Representative.
	Scanner motor failure.	Contact a Metrologic Representative.
Multiple scans upon presentation of code.	Same symbol timeout set too short.	Adjust same symbol timeout for a longer time.
The unit powers up but does not beep.	Beeper disabled No volume is selected No tone is selected.	Enable beeper Select volume (programmable) Select tone.

SYMPTOMS	POSSIBLE CAUSE(S)	SOLUTION
The unit powers up, but does not scan and/or beep.	Scanning a particular symbology that is not enabled.	UPC/EAN, Code 39, interleaved 2 of 5, Code 93, Code 128 and Codabar are enabled by default. Verify that the type of bar code being read has been selected.
	The scanner has been programmed for a character length lock, or a minimum length and bar code being scanned does not satisfy the programmed criteria.	Verify that the bar code that is being scanned falls into the criteria. (Typical of Non-UPC/EAN codes. *The scanner defaults to a minimum of 4 character bar code.*)
The unit scans a bar code, but locks up after the first scan (red LED stays on).	The scanner is configured to support some form of host handshaking but is not receiving the signal.	If the scanner is setup to support ACK/NAK, RTS/CTS, XON/XOFF or D/E, verify that the host cable and host are supporting the handshaking properly.
The unit scans, but the data transmitted to the host is incorrect.	The scanner's data format does not match the host system requirements.	Verify that the scanner's data format matches that required by the host. Make sure that the scanner is connected to the proper host port.
Scanner beeps at some bar codes and NOT for others of the same bar code symbology.	The print quality of the bar code is suspect.	Check print mode. The type of printer could be the problem. Change print settings. For example change to econo mode or high speed.
	Also check character length lock.	
	The aspect ratio of the bar code is out of tolerance.	

SYMPTOMS	POSSIBLE CAUSE(S)	SOLUTION
Scanner beeps at some bar codes and NOT for others of the same bar code symbology.	The bar code may have been printed incorrectly.	Check if it is a check digit/character/or border problem.
	The scanner is not configured correctly for this type of bar code.	Check if check digits are set properly.
	The minimum symbol length setting does not work with the bar code.	Check if the correct minimum symbol length is set.
Multi-Function Button is not working.	Dirt could be preventing the button from compressing fully.	Make sure the button area is clean and the button can move freely.
	A faulty push button switch.	Contact a Metrologic Customer Service Representative.
Keyboard Wedge Only		
The unit scans the bar code but there is no data.	Configuration is not correct.	Make sure the scanner is configured for the appropriate mode.
The unit scans but the data is not correct.	Configuration is not correct.	Make sure that the proper PC type AT, PS2 or XT is selected. Verify correct country code and data formatting are selected. Adjust the intercharacter delay SYMPTOM.
The unit is transmitting each character.	Configuration is not correct.	Increase the interscan code delay setting. Adjust whether the F0 break is transmitted. It may be necessary to try this in both settings.
Alpha characters show as lower case.	Computer is in Caps Lock mode.	Enable Caps Lock detect setting of the scanner to detect whether the PC is operating in Caps Lock.

SYMPTOMS	POSSIBLE CAUSE(S)	SOLUTION
Everything works except for a couple of characters.	These characters may not be supported by that country's key look up table.	Try operating the scanner in Alt mode.
RS-232 Only		
The unit is transmitting each character.	Configuration is not correct.	Increase the interscan code delay setting. Adjust whether the F0 break is transmitted. It may be necessary to try this in both settings.
Alpha characters show as lower case.	Computer is in Caps Lock mode.	Enable the caps lock detect setting of the scanner to detect if the PC is operating in Caps Lock.
Everything works except for a couple of characters.	These characters may not be supported by that country's key look up table.	Try operating the scanner in Alt mode.
Power-up OK and scans OK but does not communicate properly to the host.	Com port at the host is not working or configured properly.	Check to make sure that the baud rate and parity of the scanner and the communication port match and the program is looking for "RS-232" data.
	Com port not operating properly.	
	Cable not connected to the proper com port.	

SYMPTOMS	POSSIBLE CAUSE(S)	SOLUTION
The host is receiving data but the data does not look correct.	The scanner and host may not be configured for the same interface.	Check that the scanner and the host are configured for the same interface.
Characters are being dropped.	Intercharacter delay needs to be added to the transmitted output.	Add some intercharacter delay to the transmitted output by using the MetroSelect® Programming Guide (MLPN 00-02407A-1 and 00-02407A-2).
Aux Port Operation with any Interface		
Trouble with the Aux Scanner.		Refer to the user guide provided with the slave scanner.
Aux port scanner powers up but data is not relayed to the host.	Cable [MLPN 54-54667] may not be connected to the proper port.	Ensure the aux port scanner is connected to the MS7320 com port marked “Aux” port.
	The “Aux” com port may not be operating properly.	* The MS7320 must be programmed to enable the “Aux” port.
		The slave scanner must be configured to send “slave” formatted data (reserve code 32).
* Use MetroSet®. For the Auxiliary interface, choose “HoloTrak Decode”. All remaining parameters will be automatically chosen.		
USB Only		
The scanner Powers up ok, scans ok but does not communicate.	The USB Port is not operating correctly.	Check that the scanner is programmed for USB operation. Check that the host’s USB port is enabled.
The scanner emits a razz tone and the LEDS flash three times when configured for USB.	The USB port is not operating correctly.	Disconnect then reconnect the USB cable at the host end. Contact a Metrologic
		Representative if symptoms persist.

	MS7320 SERIES DESIGN SPECIFICATIONS
OPERATIONAL	
Light Source:	VLD 650 ± 10 nm
Laser Power:	0.678 mW (peak)
Depth of Field:	0 mm to 215 mm (0”- 8.5”) for 0.33 mm (13 mil) bar code
Width of Scan Field:	38 mm (1.5”) @ 15 mm (0.6”); 135 mm (5.3”) @ 191 mm (7.5”)
Scan Speed:	2000 scans/second
Scan Pattern:	5 fields of 4 parallel lines (omnidirectional)
Scan Lines:	20
Min Bar Width:	0.127 mm (5.0 mil)
Decode Capability:	Autodiscriminates all standard bar codes; for other symbologies call Metrologic
System Interfaces:	PC Keyboard Wedge, RS-232, OCIA, Light Pen, Stand Alone PC Keyboard, USB, IBM 468x/469x
Print Contrast:	35% minimum reflectance difference
No. Characters Read:	up to 80 data characters (Maximum number will vary based on symbology and density)
Roll, Pitch, Yaw:	360°, 60°, 60°
Beeper Operation:	7 tones or no beep
Indicators (LED):	green = laser on, ready to scan red = good read, decoding
MECHANICAL	
Dimensions:	185 mm (7.3") H, 99 mm (3.9") D, 168 mm (6.6") W
Footprint of Stand	64 mm (2.5”) x 64 mm (2.5”)
Weight:	1.2 Kg (2.65 lbs)
Termination:	Three 10-pin modular RJ45 jacks
Cable:	Standard 2.1m (7’) straight; for other cables call Metrologic

Specifications subject to change without notice

	MS7320 SERIES DESIGN SPECIFICATIONS
ELECTRICAL	
Input Voltage:	5.2VDC ± 0.25V
Power:	1.9 W
Operating Current:	360 mA
DC Transformers:	Class II; 5.2 VDC @ 650 mA
Class 1 Laser Product:	IEC 60825-1:1993+A1:1997+A2:2001
EMC:	FCC, ICES-003 & EN 55022 Class B
ENVIRONMENTAL	
Operating Temperature:	0°C to 40°C (32°F to 104°F)
Storage Temperature:	-40°C to 60°C (-40°F to 140°F)
Humidity:	5% to 95% relative humidity, non-condensing
Light Levels:	Up to 4842 LUX (450 foot candles)
Contaminants:	Sealed to resist airborne particulate contaminants
Ventilation:	None required

Specifications subject to change without notice

RS232 DEMONSTRATION PROGRAM

If an RS232 scanner is not communicating with your IBM compatible PC, key in the following BASIC program to test that the communication port and scanner are working. This program is for demonstration purposes only. It is only intended to prove that cabling is correct, the com port is working, and the scanner is working. If the bar code data displays on the screen while using this program, it only demonstrates that the hardware interface and scanner are working. At this point, investigate whether the application software and the scanner configuration match. If the application does not support RS-232 scanners, a software wedge program that will take RS-232 data and place it into a keyboard buffer may be needed. This program tells the PC to ignore RTS-CTS, Data Set Ready (DSR) and Data Carrier Detect (DCD) signals. If the demonstration program works and yours still does not, jumper RTS to CTS and Data Terminal Reading (DTR) to DCD and DSR on the back of your PC.

```
10      CLS
20      ON ERROR GOTO 100
30      OPEN “COM1:9600,S,7,1,CS0,DS0,CD0,LF” AS #1
35      PRINT “SCAN A FEW BAR CODES”
40      LINE INPUT #1, BARCODE$
50      PRINT BARCODE$
60      K$ = INKEY$: IF K$ = CHR$(27) THEN GOTO 32766
70      GOTO 40
100     PRINT “ERROR NO.”; ERR; “ PRESS ANY KEY TO TERMINATE.”
110     K$ = INKEY$: IF K$ = “” THEN GOTO 110
32766   CLOSE: SYSTEM
32767   END
```

The model number on each scanner includes the scanner number and factory default communications protocol.

SCANNER	VERSION IDENTIFIER	COMMUNICATION PROTOCOL(S)
7320	13	RS232, IBM 46xx, OCIA, Aux
	37	RS232, Light Pen, Keyboard Wedge, Stand-Alone Keyboard, USB, Aux

The MS7320 with Built-in PC Keyboard Wedge Interface is designed to be used for keyboard emulation only. Many RS-232 programmable functions available in other Metrologic scanners are also available as keyboard wedge functions.

The following are the most important selectable options specific to the keyboard wedge.

Keyboard Type

- ** AT (includes IBM® PS2 models 50, 55, 60, 80)
- XT
- IBM PS2 (includes models 30, 70, 8556)

Keyboard Country Type

- ** USA
- Belgium
- French
- German
- Italian
- Japan
- Spanish
- Swiss
- United Kingdom

** Refer to pages 37-42 for complete information on the factory default settings. Refer to the MetroSelect® Programming Guide (MLPN 00-02407A-1 & -2) or MetroSet® 2's help files for information on how to change the default settings.

DEFAULT SETTINGS

Many functions of the scanner can be "programmed" - that is, enabled or disabled. The scanner is shipped from the factory programmed to a set of default conditions. The default parameter of the scanner has an asterisk (*) in the charts on the following pages. If an asterisk is not in the default column then the default setting is Off or Disabled. Every communication does not support every parameter. If the communication supports a parameter listed in the charts on the following pages, a check mark will appear.

PARAMETER	DEFAULT	OCIA	RS-232	LIGHT PEN	IBM 46XX	KBW	USB
UPC/EAN	*	✔	✔	✔	✔	✔	✔
Code 128	*	✔	✔	✔	✔	✔	✔
Code 93	*	✔	✔	✔	✔	✔	✔
Codabar	*	✔	✔	✔	✔	✔	✔
Interleaved 2 of 5 (ITF)	*	✔	✔	✔	✔	✔	✔
MOD 10 Check on ITF		✔	✔	✔	✔	✔	✔
Code 11		✔	✔	✔	✔	✔	✔
Code 39	*	✔	✔	✔	✔	✔	✔
Full ASCII Code 39		✔	✔	✔	✔	✔	✔
MOD 43 Check on Code 39		✔	✔	✔	✔	✔	✔
MSI-Plessey		✔	✔	✔	✔	✔	✔
Airline (15 Digit) 2 of 5		✔	✔	✔	✔	✔	✔
Airline (13 Digit) 2 of 5		✔	✔	✔	✔	✔	✔
Matrix 2 of 5		✔	✔	✔	✔	✔	✔
Telepen		✔	✔	✔	✔	✔	✔
UK Plessey		✔	✔	✔	✔	✔	✔
STD 2 of 5		✔	✔	✔	✔	✔	✔
MSI-Plessey 10/10 Check Digit		✔	✔	✔	✔	✔	✔
MSI-Plessey MOD 10 Check Digit	*	✔	✔	✔	✔	✔	✔
Paraf Support		✔	✔	✔	✔	✔	✔
ITF Symbol Lengths	Variable	✔	✔	✔	✔	✔	✔
Minimum Symbol Length	4	✔	✔	✔	✔	✔	✔
Symbol Length Lock	None	✔	✔	✔	✔	✔	✔
Bars High as Code 39	*			✔			

Parameter	Default	OCIA	RS-232	Light Pen	IBM 46XX	KBW	USB
Spaces High as Code 39				✔			
Bars High as Scanned				✔			
Spaces High as Scanned				✔			
DTS/SIEMENS		✔					
DTS/NIXDORF	*	✔					
NCR F		✔					
NCR S		✔					
Poll Light Pen Source				✔			
Beeper Tone	Normal	✔	✔	✔	✔	✔	✔
Beep/Transmit Sequence	Before Transmit	✔	✔	✔	✔	✔	✔
Beeper Volume	Loudest	✔	✔	✔	✔	✔	✔
Communication Timeout	None	✔	✔	✔	✔	✔	✔
Razzberry Tone on Timeout		✔	✔	✔	✔	✔	✔
Three Beeps on Timeout		✔	✔	✔	✔	✔	✔
No Beeps on Timeout	*	✔	✔	✔	✔	✔	✔
Enter Power Save Mode	10 mins.	✔	✔	✔	✔	✔	✔
Blink Power Save Mode	*	✔	✔	✔	✔	✔	✔
Laser OFF Power Save Mode		✔	✔	✔	✔	✔	✔
Laser & Motor OFF Power Save Mode		✔	✔	✔	✔	✔	✔
Dual Action Power Save Mode #1		✔	✔	✔	✔	✔	✔
Dual Action Power Save Mode #2		✔	✔	✔	✔	✔	✔
Same Symbol Rescan Timeout: 200 msecs		✔	✔	✔	✔	✔	✔
Same Symbol Rescan Timeout: 500 msecs Programmable in 50 msec steps (MAX 6.35 seconds)	*	✔	✔	✔	✔	✔	✔
Same Symbol Rescan Timeout: 1250 msecs		✔	✔	✔	✔	✔	✔

DEFAULT SETTINGS (CONTINUED)

Parameter	Default	OCIA	RS-232	Light Pen	IBM 46XX	KBW	USB
Same Symbol Rescan Timeout: 2000 msecs		✔	✔	✔	✔	✔	✔
Intercharacter Delay Programmable in 1 msec steps (MAX 255 msecs)	1 msecs 10 msecs in KBW	✔	✔		✔	✔	
Number of Scan Buffers	1	✔	✔	✔	✔	✔	✔
Transmit EAN-8 Check Digit	*	✔	✔		✔	✔	✔
Transmit EAN-13 Check Digit	*	✔	✔		✔	✔	✔
Transmit UPC-A Check Digit	*	✔	✔		✔	✔	✔
Transmit UPC-E Check Digit			✔		✔	✔	✔
Expand UPC-E		✔	✔		✔	✔	✔
Convert UPC-A to EAN-13		✔	✔		✔	✔	✔
UPC GTIN-14 Format		✔	✔		✔	✔	✔
Transmit Lead Zero on UPC-E		✔	✔	✔	✔	✔	✔
Convert EAN-8 to EAN-13		✔	✔		✔	✔	✔
Transmit UPC-A Number System	*	✔	✔	✔	✔	✔	✔
Transmit UPC-A Manufacturer ID#	*	✔	✔	✔	✔	✔	✔
Transmit UPC-A Item ID#	*	✔	✔	✔	✔	✔	✔
Transmit Codabar Start/Stop Characters		✔	✔		✔	✔	✔
CLSI Editing (Enable)		✔	✔		✔	✔	✔
Transmit Mod 43 Check Digit on Code 39		✔	✔		✔	✔	✔
Transmit Code 39 Stop/Start Characters		✔	✔		✔	✔	✔
Transmit Mod 10/ITF		✔	✔		✔	✔	✔
Transmit MSI-Plessey Check Characters		✔	✔		✔	✔	✔
Parity	Space		✔				
Baud Rate	9600		✔				

Parameter	Default	OCIA	RS-232	Light Pen	IBM 46XX	KBW	USB
8 Data Bits			✔				
7 Data Bits	*		✔				
Transmit Sanyo ID Characters			✔			✔	✔
Nixdorf ID			✔			✔	✔
LRC Enabled			✔			✔	✔
UPC Prefix			✔			✔	✔
UPC Suffix			✔			✔	✔
Transmit AIM ID Characters			✔			✔	✔
STX Prefix			✔			✔	✔
ETX Suffix			✔			✔	✔
Carriage Return	*		✔			✔	✔
Line Feed - disabled by default in KBW	*		✔			✔	✔
Tab Prefix			✔			✔	✔
Tab Suffix			✔			✔	✔
"DE" Disable Command			✔				✔
"FL" Laser Enable Command			✔				✔
DTR Handshaking Support			✔				
RTS/CTS Handshaking			✔				
Character RTS/CTS	*		✔				
Message RTS/CTS			✔				
XON/XOFF Handshaking			✔				
ACK/NAK			✔				
Two Digit Supplements		✔	✔	as code 39	✔	✔	✔
Five Digit Supplements		✔	✔	as code 39	✔	✔	✔
Bookland 978		✔	✔	as code 39	✔	✔	✔

Parameter	Default	OCIA	RS-232	Light Pen	IBM 46XX	KBW	USB
Bookland 977 (2 digit) Supplemental Requirement		✔	✔	✔	✔	✔	✔
Supplements are not Required	*	✔	✔	✔	✔	✔	✔
Two Digit Redundancy	*	✔	✔	✔	✔	✔	✔
Five Digit Redundancy		✔	✔	✔	✔	✔	✔
100 msec to Find Supplement Programmable in 100 msec steps (MAX 800 msec)	*	✔	✔	✔	✔	✔	✔
Coupon Code 128		✔	✔	as code 39	✔	✔	✔
Programmable Code Lengths	7 avail.	✔	✔	✔	✔	✔	✔
Programmable Prefix Characters	10 avail.		✔			✔	✔
Suffix Characters			✔			✔	✔
Prefixes for individual Code Types			✔			✔	✔
Editing		✔	✔	✔	✔	✔	✔
Inter Scan-Code Delay Programmable (100 µsec steps)	800 µsec					✔	✔
Function/Control Key Support						✔	✔
Minimum Element Width Programmable in 5.6 µsec steps	1 msec			✔			
Depth of Field							
Variable Depth of Field	*	✔	✔	✔	✔	✔	✔
Normal Depth of Field	*	✔	✔	✔	✔	✔	✔
Extended Depth of Field		✔	✔	✔	✔	✔	✔
Long Depth of Field	*	✔	✔	✔	✔	✔	✔
Ultra Close Depth of Field		✔	✔	✔	✔	✔	✔

Default settings for "*Aux*" interface

The slave scanner and the MS7320 always communicate via RS232. Data is relayed to the host via various primary interfaces.

Parameter	Default	OCIA	RS-232	Light Pen	IBM 46XX	KBW	USB
Aux Baud Rate	38400	✔	✔	✔	✔	✔	✔
Aux parity	space	✔	✔	✔	✔	✔	✔
Aux data bits	7	✔	✔	✔	✔	✔	✔
Aux stop bits	2	✔	✔	✔	✔	✔	✔
Aux character RTS	*	✔	✔	✔	✔	✔	✔
Aux message RTS		✔	✔	✔	✔	✔	✔
Aux Ack/Nak	*	✔	✔	✔	✔	✔	✔
Aux Xon/Xoff	*	✔	✔	✔	✔	✔	✔
Aux D/E commands		✔	✔	✔	✔	✔	✔
Aux M/O commands		✔	✔	✔	✔	✔	✔
Aux F/L commands		✔	✔	✔	✔	✔	✔
Aux Intercharacter Delay	1 msec	✔	✔	✔	✔	✔	✔
Aux Port Data Format	None (Disabled)	✔	✔	✔	✔	✔	✔

Scanner Pinout Connections

The MS7320 scanner interfaces terminate to 10-pin modular jacks located on the back of the unit. The serial # label indicates the model number of the scanner.

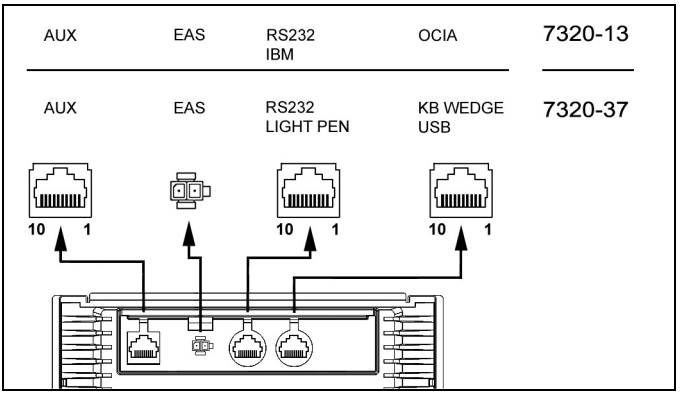

Figure 28: *Scanner Interface Ports*

MS732x-13 OCIA	
Pin	**Function**
1	Ground
2	NC
3	NC
4	RDATA
5	RDATA Return
6	Clock in
7	Clock out
8	Clock in Return/ Clock out Rtrn
9	+5VDC
10	Shield Ground

MS732x-13 IBM 46xx	
Pin	**Function**
1	Ground
2	RS-232 Transmit Output
3	RS-232 Receive Input
4	RTS Output
5	CTS Input
6	DTR
7	IBM B- (D-)
8	IBM A+ (D+)
9	+5V IN
10	NC

Continued next page

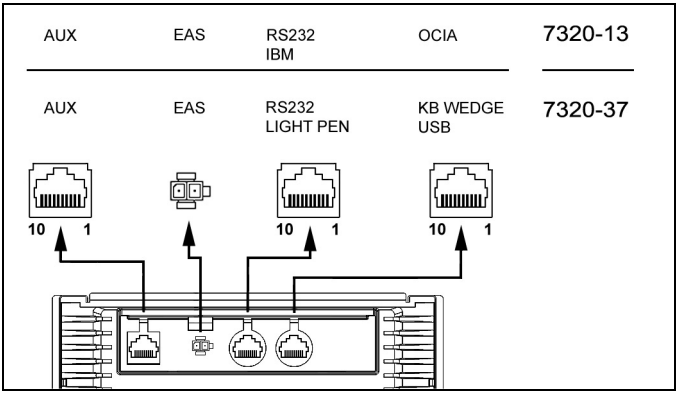

Figure 29: *Scanner Interface Ports*

MS732x-37 Keyboard Wedge, Stand Alone-Keyboard or USB	
Pin	**Function**
1	Ground
2	USB D-
3	USB D+
4	PC Data
5	PC Clock
6	KB Clock
7	PC +5V, V-USB
8	KB Data
9	+5VDC
10	Shield Ground

MS732x-37 RS-232 or Light Pen	
Pin	**Function**
1	Ground
2	RS-232 Transmit Output
3	RS-232 Receive Input
4	RTS Output
5	CTS Input
6	DTR Input/LTPN Source
7	N/C
8	LTPN Data
9	+5VDC
10	Shield Ground

MS732x-13/-37 Auxilary Port RS232 IN Only	
Pin	**Function**
1	Ground
2	RS-232 Receive Input
3	RS-232 Transmit Output
4	RTS In
5	CTS Out
6-10	NC

Cable Connector Configurations (Host End)

PowerLink Cable MLPN 54-54xxx*	
Pin	**Function**
1	Shield Ground
2	RS-232 Transmit Output
3	RS-232 Receive Input
4	DTR Input
5	Power/Signal Ground
6	Reserved
7	CTS Input
8	RTS Output
9	+5VDC



9-Pin D-Type Conn.

xxx* specifies connection to the host

USB PowerLink Cable (MLPN 54-54165, Type A)	
Pin	**Function**
1	N/C
2	D-
3	D+
4	Ground



USB Type A (Top)
Locking Type A (Bottom)



PowerLink, RS232 AUX Cable MLPN 54-54667	
Pin	**Function**
1	Ground
2	RS-232 Transmit Output
3	RS-232 Receive Input
4	RTS Output
5	CTS Input
6-10	N/C



10-pin Modular Plug

Stand Alone Keyboard Cable MLPN 54-54020	
Pin	**Function**
1	PC Data
2	NC
3	Power Ground
4	+5VDC PC Power to KB
5	PC Clock
6	NC



6-Pin Male Mini-DIN Conn.

Cable Connector Configuration

The PowerLink cable is terminated with a 5-pin DIN female connector on one end, and a 6-pin mini DIN male on the other.



PowerLink Cable

5-Pin DIN, Female



6-Pin DIN, Male

Metrologic will supply an adapter cable with a 5-pin DIN male connector on one end and a 6-pin mini DIN female connector on the other.



5-Pin Din, Male

Adapter Cable



6-pin Mini Din, Female

According to the termination required, connect the appropriate end of the adapter cable to the PowerLink cable, leaving the necessary termination exposed for connecting to the keyboard and the keyboard port on the PC. The pin assignments are as follows:

PowerLink Cable	
5-pin Female DIN	
Pin	**Function**
1	Keyboard Clock
2	Keyboard Data
3	No Connect
4	Power Ground
5	+5 Volts DC
6-pin Male Mini-DIN	
Pin	**Function**
1	Keyboard Data
2	No Connect
3	Power Ground
4	+5 Volts DC
5	PC Clock
6	No Connect

Adapter Cable	
5-pin Male DIN	
Pin	**Function**
1	PC Clock
2	PC Data
3	No Connect
4	Power Ground
5	+5 Volts DC
6-pin Female Mini-DIN	
Pin	**Function**
1	Keyboard Data
2	No Connect
3	Power Ground
4	+5 Volts DC
5	Keyboard Clock
6	No Connect

LIMITED WARRANTY

The MS7320 InVista™ Series scanners are manufactured by Metrologic at its Blackwood, New Jersey, U.S.A. facility. The MS7320 Series scanners have a two (2) year limited warranty from the date of manufacture. Metrologic warrants and represents that all MS7320 Series scanners are free of all defects in material, workmanship and design, and have been produced and labeled in compliance with all applicable U.S. Federal, state and local laws, regulations and ordinances pertaining to their production and labeling.

This warranty is limited to repair, replacement of Product or refund of Product price at the sole discretion of Metrologic. Faulty equipment must be returned to the Metrologic facility in Blackwood, New Jersey, U.S.A. or Puchheim, Germany. To do this, contact Metrologic's Customer Service/Repair Department to obtain a Returned Material Authorization (RMA) number.

In the event that it is determined the equipment failure is covered under this warranty, Metrologic shall, at its sole option, repair the Product or replace the Product with a functionally equivalent unit and return such repaired or replaced Product without charge for service or return freight, whether distributor, dealer/reseller, or retail consumer, or refund an amount equal to the original purchase price.

This limited warranty does not extend to any Product which, in the sole judgement of Metrologic, has been subjected to abuse, misuse, neglect, improper installation, or accident, nor any damage due to use or misuse produced from integration of the Product into any mechanical, electrical or computer system. The warranty is void if the case of Product is opened by anyone other than Metrologic's repair department or authorized repair centers.

THIS LIMITED WARRANTY, EXCEPT AS TO TITLE, IS IN LIEU OF ALL OTHER WARRANTIES OR GUARANTEES, EITHER EXPRESS OR IMPLIED, AND SPECIFICALLY EXCLUDES, WITHOUT LIMITATION, WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE UNDER THE UNIFORM COMMERCIAL CODE, OR ARISING OUT OF CUSTOM OR CONDUCT. THE RIGHTS AND REMEDIES PROVIDED HEREIN ARE EXCLUSIVE AND IN LIEU OF ANY OTHER RIGHTS OR REMEDIES. IN NO EVENT SHALL METROLOGIC BE LIABLE FOR ANY INDIRECT OR CONSEQUENTIAL DAMAGES, INCIDENTAL DAMAGES, DAMAGES TO PERSON OR PROPERTY, OR EFFECT ON BUSINESS OR PROPERTY, OR OTHER DAMAGES OR EXPENSES DUE DIRECTLY OR INDIRECTLY TO THE PRODUCT, EXCEPT AS STATED IN THIS WARRANTY. IN NO EVENT SHALL ANY LIABILITY OF METROLOGIC EXCEED THE ACTUAL AMOUNT PAID TO METROLOGIC FOR THE PRODUCT. METROLOGIC RESERVES THE RIGHT TO MAKE ANY CHANGES TO THE PRODUCT DESCRIBED HEREIN.

Corporate Headquarters

Metrologic Instruments, Inc.
90 Coles Road
Blackwood, NJ 08012-4683

Customer Service: 1-800-ID-METRO
Tel: 856-228-8100
Fax: 856-228-6673
Email: info@metrologic.com
Website: www.metrologic.com

Germany

Metrologic Instruments GmbH
Dornierstrasse 2
82178 Puchheim b.
Munich, Germany

Tel: 49-89-89019-0
Fax: 49-89-89019-200
Email: info@europe.metrologic.com

NOTICES

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna
- Increase the separation between the equipment and receiver
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected
- Consult the dealer or an experienced radio/TV technician for help

Notice
This Class B digital apparatus complies with Canadian ICES-003.

Avertissement
Cet appareil numérique de la class B est conforme à la norme NMB-003.

⚠Caution
Use of controls or adjustments or performance of procedures other than those specified herein may result in hazardous laser light exposure. Under no circumstances should the customer attempt to service the laser scanner. Never attempt to look at the laser beam, even if the scanner appears to be nonfunctional. Never open the scanner in an attempt to look into the device. Doing so could result in hazardous laser light exposure. The use of optical instruments with the laser equipment will increase eye hazard.

⚠Atención
La modificación de los procedimientos, o la utilización de controles o ajustes distintos de los especificados aquí, pueden provocar una luz de láser peligrosa. Bajo ninguna circunstancia el usuario deberá realizar el mantenimiento del láser del escáner. Ni intentar mirar al haz del láser incluso cuando este no esté operativo. Tampoco deberá abrir el escáner para examinar el aparato. El hacerlo puede conllevar una exposición peligrosa a la luz de láser. El uso de instrumentos ópticos con el equipo láser puede incrementar el riesgo para la vista.

⚠Attention
L'emploi de commandes, réglages ou procédés autres que ceux décrits ici peut entraîner de graves irradiations. Le client ne doit en aucun cas essayer d'entretenir lui-même le scanner ou le laser. Ne regardez jamais directement le rayon laser, même si vous croyez que le scanner est inactif. N'ouvrez jamais le scanner pour regarder dans l'appareil. Ce faisant, vous vous exposez à une rayonnement laser qú êst hazardous. L'emploi d'appareils optiques avec cet équipement laser augmente le risque d'endommagement de la vision.

⚠Achtung
Die Verwendung anderer als der hier beschriebenen Steuerungen, Einstellungen oder Verfahren kann eine gefährliche Laserstrahlung hervorrufen. Der Kunde sollte unter keinen Umständen versuchen, den Laser-Scanner selbst zu warten. Sehen Sie niemals in den Laserstrahl, selbst wenn Sie glauben, daß der Scanner nicht aktiv ist. Öffnen Sie niemals den Scanner, um in das Gerät hineinzusehen. Wenn Sie dies tun, können Sie sich einer gefährlichen Laserstrahlung aussetzen. Der Einsatz optischer Geräte mit dieser Laserausrüstung erhöht das Risiko einer Sehschädigung.

⚠Attenzione
L'utilizzo di sistemi di controllo, di regolazioni o di procedimenti diversi da quelli descritti nel presente Manuale può provocare delle esposizioni a raggi laser rischiose. Il cliente non deve assolutamente tentare di riparare egli stesso lo scanner laser. Non guardate mai il raggio laser, anche se credete che lo scanner non sia attivo. Non aprite mai lo scanner per guardare dentro l'apparecchio. Facendolo potete esporVi ad una esposizione laser rischiosa. L'uso di apparecchi ottici, equipaggiati con raggi laser, aumenta il rischio di danni alla vista.

PATENTS

“Patent Information

This METROLOGIC product may be covered by one or more of the following U.S. Patents:

U.S. Patent No.;
4,960,985; 5,081,342; 5,216,232; 5,557,093; 5,627,359; 5,637,852;
5,661,292; 5,777,315; 5,789,731; 6,029,894; 6,098,885; 6,209,789;

4,360,798; 4,369,361; 4,387,297; 4,460,120; 4,496,831; 4,593,186;
4,607,156; 4,673,805; 4,736,095; 4,758,717; 4,816,660; 4,845,350;
4,896,026; 4,923,281; 4,933,538; 4,992,717; 5,081,342; 5,015,833;
5,017,765; 5,059,779; 5,117,098; 5,124,539; 5,130,520; 5,132,525;
5,140,144; 5,149,950; 5,180,904; 5,200,599; 5,229,591; 5,247,162;
5,250,790; 5,250,791; 5,250,792; 5,260,553; 5,262,628; 5,280,162;
5,280,164; 5,304,788; 5,321,246; 5,324,924; 5,340,973; 5,396,053;
5,396,055; 5,408,081; 5,410,139; 5,424,525; 5,436,440; 5,449,891;
5,468,949; 5,468,951; 5,479,000; 5,484,992; 5,525,789; 5,528,024;
5,532,469; 5,545,889; 5,591,953; 5,616,908; 5,627,359;

No license right or sublicense is granted, either expressly or by implication, estoppel, or otherwise, under any METROLOGIC or third party intellectual property rights (whether or not such third party rights are licensed to METROLOGIC), including any third party patent listed above, except for an implied license only for the normal intended use of the specific equipment, circuits, and devices represented by or contained in the METROLOGIC products that are physically transferred to the user, and only to the extent of METROLOGIC’S license rights and subject to any conditions, covenants and restrictions therein.”

Other worldwide patents pending.

A
Accessories 2
Adapter 46
Audible.....17
Autodiscriminates 33

B
Bar Code 22, 23, 24
Beep 17, 38
Button 21

C
Cable 2, 8, 14, 31-33, 43-46
Cable Cover.....15
Caution 4, 5, 6, 7, 8, 10, 11
CE.....49
Communication.....36, 38
Connector 45, 46
Customer Service 3, 47

D
Decode Capability 33
Default Settings 37-42
Design Specifications 33, 34

E
EAS 27
Electrical 34
Extended Depth of Field 41

F
Face Plate 15
Failure Modes 19
Function..... 41, 43-46

G
Ground..... 43-46

H
Host 11

I
Indicators 17, 18, 33
Input Voltage 34
Installation 4, 5, 7-13
Interfaces..... 4, 6-10, 28

K
Keyboard Type 36
Keyboard Wedge 1, 2, 5, 33, 36, 44

L
Labels.....16
LED 14, 17, 18, 28, 29, 33
Light Levels 34
Light Pen 1, 8-10, 33, 36-42, 44
Light Source 33

M
Maintenance.....14
Mechanical 33
Min Bar Width.....33
Modes 20
Multi-Function Button 21

N
Normal Depth of Field 41
Notices 48, 49

O
OCIA 4, 33, 37-43
Operating Current 34
Operation 33
Operational.....33
Output Window..... 14

P
Parts..... 14
Patents 50
Port..... 42, 44
Power Save 20
Programming Guide 32, 36
Protocols 36

R
Razzberry Tone..... 17, 19, 38
RDATA 43
Repair.....47

S
Scan Lines 33
Scan Pattern 33
Scan Speed.....33

Specifications 22-24, 33, 34
Stand 25, 26, 33
Storage 34
System Interfaces 33

T
Termination.....33
Transformers 34
Troubleshooting...28, 29, 30, 31, 32

U
USB 7

V
Ventilation 34
Visual 18
Voltage 4, 5, 6, 7, 8, 10, 11

W
Warranty 47
Weight.....33
Window Cover.....14

April 2002

Printed in the USA

00-02896A